


# ACCU-Beam® Universal Video EndoAdaptor

Product No. 8012

## User Instructions

The ACCU-Beam® Universal Video EndoAdaptor is a precision optical instrument and should be handled with care. A 30mm lens provides optimal light transmission, color correction and a flat field image. The eyepiece clamp will accommodate a standard 32mm eyepiece.

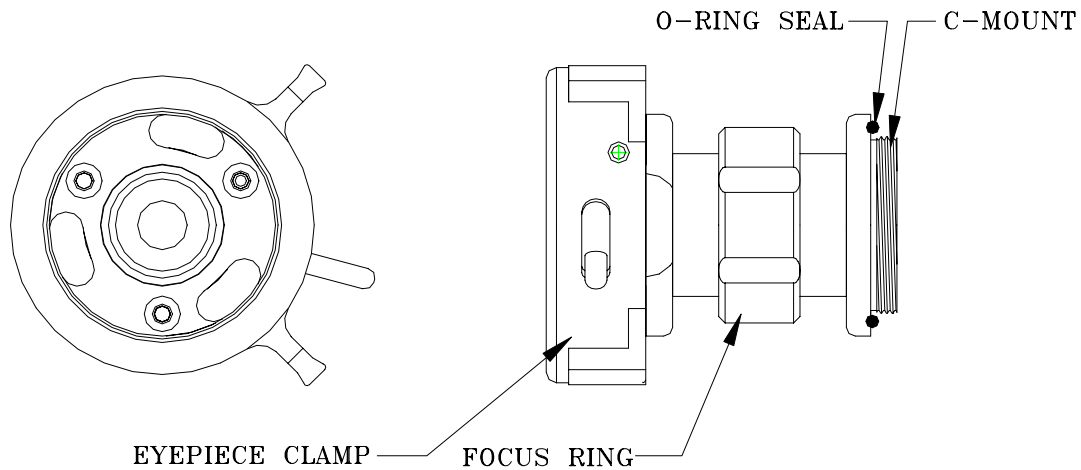

**TRANSAMERICAN TECHNOLOGIES INTERNATIONAL**

**2246 Camino Ramon • San Ramon • CA 94583 USA**

**Tel: 925-355-0750 • 800-322-7373 • Fax: 925-355-0777**

## **Mounting the Camera:**

- 1. The ACCU-Beam®EndoAdaptor screws into the c-mount thread of the video camera. *CAUTION – do not over tighten.* The o-ring seal at the base of the c-mount thread creates a water tight seal between the camera and the adaptor.**

## **Mounting the Endoscope:**

- 1. The eyepiece of the endoscope fits into the eyepiece clamp by moving the clamp lever to the open position, load the eyepiece and release.**
- 2. Even through the endoscope is firmly held in place, it can easily be rotated with the opposite hand. This may be necessary when using an angle viewing scope such as a 30° endoscope.**
- 3. To lock the endoscope, move the clamping lever to the lock position as far as possible and release. To unlock, move the clamping lever to the open position.**

**Focusing:** With illumination on, point the distal end of the endoscope at a target about 10cm away and turn the focus ring until the video image is in sharp focus.

## **Cleaning, Disinfecting and Sterilization:**

- 1. The Video EndoAdaptor is completely sealed, however it is recommended that the Camera Head and EndoAdaptor are to be attached for cleaning, disinfecting and sterilization. They should be threaded together until hand tight and their o-ring seals compressed. If they are soaked or sterilized apart, special care must be taken afterwards to ensure the Camera Head and EndoAdaptor interface is completely dry prior to attachment or fogging may occur.**

2. **Cleaning** – Thoroughly clean with soap and water – then rinse. If the window requires additional cleaning, use lens paper or a soft cotton swab (without adhesive) dipped in reagent grade acetone. Optics should be cleaned in a circular motion from the center to the outside. **CAUTION** – *Do not use alcohol or other cleaning agents on lenses.*
  
3. **Soak Disinfecting** – Using 2% activated glutaraldehyde solution, soak for 20 minutes at 20°C (68°F). Rinse 3 times with sterile water to remove residual glutaraldehyde. Use separate containers for each rinse. **CAUTION** – *Residual glutaraldehyde can be harmful to tissue causing chemical burns.*
  
4. **Sterilization** – Steris, Sterrad or ETO. Note - After sterilization, wipe any moisture off the EndoAdaptor window with a sterile swab before mounting the endoscope to prevent fogging. **CAUTION** – *Do not autoclave*
  
5. **Sterile Drapes** – Disposable sterile drapes may be used to provide a sterile barrier around the EndoAdaptor, camera head and camera cable.

**Authorized Representative per Medical Device Directive  
Hallmark International Management Consultants  
Systems House, Westgate, Tadcaster  
North Yorkshire LS24 9AA, UK**

ISO9001:1994  
AMTAC Cert No. 163



**TRANSAMERICAN TECHNOLOGIES INTERNATIONAL**  
2264 Camino Ramon • San Ramon • CA 94583 USA  
Tel: 925-355-0750 • 800-322-7373 • Fax: 925-355-  
0777

e-mail: [ttimed@aol.com](mailto:ttimed@aol.com) • website:  
www.ttimedical.com